

The variable finesse locking technique

F Acernese¹, P Amico², M Al-Shourbagy³, S Aoudia⁴, S Avino¹,
 D Babusci⁵, G Ballardin⁶, R Barillé⁶, F Barone¹, L Barsotti³,
 M Barsuglia⁷, F Beauville⁸, M A Bizouard⁷, C Boccara⁹, F Bondu⁴,
 L Bosi², C Bradaschia³, S Braccini³, A Brilliet⁴, V Brisson⁷, L Brocco¹⁰,
 D Buskulic⁸, E Calloni¹, E Campagna¹¹, F Cavalier⁷, R Cavalieri⁶,
 G Cella³, E Chassande-Mottin⁴, C Corda³, A-C Clapson⁷, F Cleva⁴,
 J-P Coulon⁴, E Cuoco⁶, V Dattilo⁶, M Davier⁷, R De Rosa¹, L Di Fiore¹,
 A Di Virgilio³, B Dujardin⁴, A Eleuteri¹, D Enard⁶, I Ferrante³,
 F Fidecaro^{3,6}, I Fiori³, R Flaminio^{6,8}, J-D Fournier⁴, S Frasca¹⁰,
 F Frasconi^{3,6}, A Freise⁶, L Gammaitoni², A Gennai³, A Giazotto³,
 G Giordano⁵, L Giordano¹, R Gouaty⁸, D Grosjean⁸, G Guidi¹¹, S Hebré⁶,
 H Heitmann⁴, P Hello⁷, L Holloway⁶, S Kreckelbergh⁷, P La Penna⁶,
 V Lorientte⁹, M Loupias⁶, G Losurdo¹¹, J-M Mackowski¹², E Majorana¹⁰,
 C N Man⁴, M Mantovani³, F Marchesoni², F Marion⁸, J Marque⁶,
 F Martelli¹¹, A Masserot⁸, M Mazzone¹¹, L Milano¹, C Moins⁶,
 J Moreau⁹, N Morgado¹², B Mours⁸, A Pai¹⁰, C Palomba¹⁰, F Paoletti^{3,6},
 S Pardi¹, A Pasqualetti⁶, R Passaquieti³, D Passuello³, B Perniola¹¹,
 F Piergiovanni¹¹, L Pinard¹², R Poggiani³, M Punturo², P Puppo¹⁰,
 K Qipiani¹, P Rapagnani¹⁰, V Reita⁹, A Remillieux¹², F Ricci¹⁰,
 I Ricciardi¹, P Ruggi⁶, G Russo¹, S Solimeno¹, A Spallicci⁴, R Stanga¹¹,
 R Taddei⁶, D Tombolato⁸, M Tonelli³, A Toncelli³, E Tournefier⁸,
 F Travasso², G Vajente³, D Verkindt⁸, F Vetrano¹¹, A Viceré¹¹, J-Y Vinet⁴,
 H Vocca², M Yvert⁸, Z Zhang⁶ and M Evans¹³

¹ INFN, Sezione di Napoli and/or Università di Napoli 'Federico II' Complesso Universitario di Monte S. Angelo, and/or Università di Salerno, Fisciano (Sa), Italy

² INFN, Sezione di Perugia and/or Università di Perugia, Perugia, Italy

³ INFN, Sezione di Pisa and/or Università di Pisa, Pisa, Italy

⁴ Département Artemis—Observatoire de la Côte d'Azur, BP 42209 06304 Nice, Cedex 4, France

⁵ INFN, Laboratori Nazionali di Frascati, Frascati (Rm), Italy

⁶ European Gravitational Observatory (EGO), Cascina (Pi), Italy

⁷ Laboratoire de l'Accélérateur Linéaire (LAL), IN2P3/CNRS-Univ. de Paris-Sud, Orsay, France

⁸ Laboratoire d'Annecy-le-Vieux de Physique des Particules, Annecy-le-Vieux, France

⁹ ESPCI, Paris, France

¹⁰ INFN, Sezione di Roma and/or Università 'La Sapienza', Roma, Italy

¹¹ INFN, Sezione di Firenze/Urbino, Sesto Fiorentino, and/or Università di Firenze, and/or Università di Urbino, Italy

¹² LMA, Villeurbanne, Lyon, France

¹³ LIGO Laboratory, California Institute of Technology, Pasadena, CA, USA

E-mail: lisa.barsotti@ego-gw.it

Received 29 August 2005

Published 24 March 2006

Online at stacks.iop.org/CQG/23/S85

Abstract

Virgo is a power recycled Michelson interferometer, with 3 km long Fabry–Perot cavities in the arms. The locking of the interferometer has been obtained with an original lock acquisition technique. The main idea is to lock the instrument away from its working point. Lock is obtained by misaligning the power recycling mirror and detuning the Michelson from the dark fringe. In this way, a good fraction of light escapes through the antisymmetric port and the power build-up inside the recycling cavity is extremely low. The benefit is that all the degrees of freedom are controlled when they are almost decoupled, and the linewidth of the recycling cavity is large. The interferometer is then adiabatically brought on to the dark fringe. This technique is referred to as variable finesse, since the recycling cavity is considered as a variable finesse Fabry–Perot. This technique has been widely tested and allows us to reach the dark fringe in few minutes, in an essentially deterministic way.

PACS numbers: 04.80.Nn, 95.55.Ym

(Some figures in this article are in colour only in the electronic version)

1. The Virgo longitudinal control system

The nominal sensitivity of a power recycled Michelson interferometer detector with suspended optics such as Virgo is achieved by selecting an appropriate working point, with laser light resonant in the optical cavities, and the output port tuned on the dark fringe. These conditions translate into fixed relationships between the laser light wavelength and four independent lengths of the interferometer (see figure 1):

- the length of the recycling cavity (PRCL), $l_{\text{rec}} + \frac{l_N + l_W}{2}$;
- the differential length of the short Michelson arms (MICH), $l_N - l_W$;
- the common (CARM) and the differential (DARM) length of the two long arms, $L_N + L_W$ and $L_N - L_W$.

The Virgo suspension system, the so-called superattenuator (SA) [1], provides very good seismic isolation in the frequency band used for detection, but below a few hertz some seismic noise is transferred to the mirrors or even amplified by the SA mechanical resonances. While the expected sensitivity is of the order of 10^{-18} m Hz^{-1/2} at the rate of 10 Hz, the allowed deviation from the working point, or locking accuracy, is 10^{-12} m rms. An active *feedback control system* is therefore needed to keep the interferometer locked on the required interference conditions.

Relative displacement of the mirrors is detected using a carrier beam phase modulated at $f = 6$ MHz. The carrier beats with the sidebands, producing light modulated in intensity with frequency $f, 2f, \dots$. Using a standard Pound–Drever–Hall scheme [2, 3] all the lengths involved can be reconstructed by mixing the signals produced by the photodiodes, which are placed at different output ports of the interferometer. These error signals are digitized and sent to the Virgo global control system (Global Control [4]), which computes the corrections to be applied to the mirrors by coil magnet actuators. A *local control system*, referred to as the ground, is active in the bottom part of each SA in order to keep the longitudinal displacement of the mirrors below $1 \mu\text{m}$ rms. In this way, the longitudinal lock of the interferometer can be acquired using a limited actuation force, thus preventing noise reinjection in the detection band.

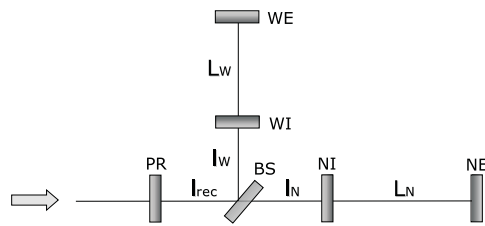


Figure 1. Optical scheme of Virgo.

2. Lock acquisition of the recycled interferometer

The process by which an interferometer in an initially uncontrolled condition is brought to and kept at its working point by closing the feedback loops is called *lock acquisition*.

Detectors with an optical set-up similar to Virgo, such as LIGO and TAMA, apply a lock acquisition technique based on a statistical approach, where the control loops are engaged every time the interferometer passes through the relative resonance conditions. The four independent lengths of the interferometer are then sequentially locked at their operating points, dynamically changing the optical sensing matrix in order to compensate the variation of the fields in the course of lock acquisition [6]. The locked state is reached in a sequence of three steps¹⁴ starting from the uncontrolled condition, where only the final one is stable.

2.1. The variable finesse locking technique

An alternative lock acquisition technique has been developed in Virgo: it differs from the multi-steps scheme mainly because all four longitudinal degrees of freedom of the interferometer are locked simultaneously.

The main idea is that the interferometer is locked away from the working point of the dark fringe. A good fraction of light escapes through the antisymmetric port and the power build-up inside the recycling cavity is extremely low. In this way, all the lengths of the interferometer are controlled when they are almost decoupled and the linewidth of the recycling cavity is large, making the control design easier. From this stable state, the interferometer is then adiabatically brought on to the dark fringe. This technique is referred to as *variable finesse*, because the finesse of the recycling cavity changes during the lock acquisition path.

2.2. The variable finesse locking procedure

The locking procedure starts with the PR mirror slightly misaligned by some microradians, in order to further decrease the power stored inside the recycling cavity. The simple Michelson is kept at mid-fringe (50% reflected, 50% transmitted), adding an offset in the dark port dc signal and applying the correction to the BS mirror. Since all the degrees of freedom are almost decoupled in this state, the two arms can be independently locked using the end photodiodes. The small quantity of light reflected by the interferometer is used to control the recycling cavity power length, by the reflected $3f$ -demodulated signal, as comprehensively tested in the TAMA control scheme [7]. This stable configuration can usually be reached

¹⁴ In the first step, the sidebands enter in resonance in the recycling cavity (anti-resonant in the arms), the carrier is on the anti-resonance for the recycling cavity and for the arms; in the second step, the carrier enters in resonance in one arm, on the bright fringe in the recycling cavity, where the sidebands remain in the same condition; in the last step, the carrier goes in resonance in both arms and in the recycling cavity [5].

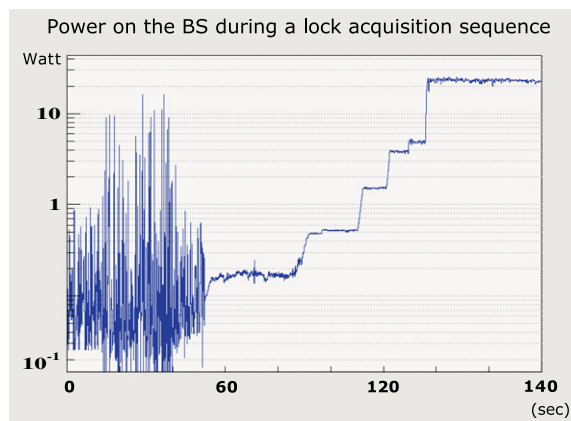


Figure 3. Lock acquisition sequence, looking at the power impinging on the BS: the interferometer is brought from the uncontrolled to the fully controlled state in less than 2 min.

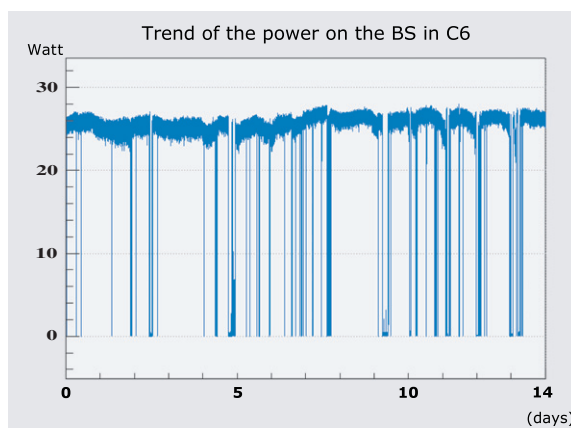


Figure 4. Trend of the power impinging on the BS during 14 days of data taking (C6): the duty cycle is around 86%.

References

- [1] Ballardin G *et al* 2001 Measurement of the VIRGO superattenuator performance for seismic noise suppression *Rev. Sci. Instrum.* **72** 3643–52
- [2] Pound R V 1946 Electronic frequency stabilization of microwave oscillators *Rev. Sci. Instrum.* **17** 490–505
- [3] Drever R W P *et al* 1983 Laser phase and frequency stabilization using an optical resonator *Appl. Phys. B* **31** 97–105
- [4] Cavalier F 2001 Le controle global de Virgo *These d'Habilitation a diriger des Recherches* Université de Paris Sud, LAL 01-69
- [5] Evans M 2001 Lock acquisition in resonant optical interferometers *PhD Thesis* CALTECH
- [6] Evans M *et al* 2002 Lock acquisition of a gravitational-wave interferometer *Opt. Lett.* **27** 598–600
- [7] Arai K (TAMA Collaboration) 2002 Sensing and controls for power-recycling of TAMA300 *Class. Quantum Grav.* **19** 1843–8
- [8] Arai K 2001 Robust extraction of control signals for power-recycled interferometric gravitational-wave detectors *PhD Thesis* University of Tokyo
- [9] Acernese F *et al* 2006 *Class. Quantum Grav.* **23** S63